



BEST AVAILABLE COPY

partially occluded stereoscopic displayed objects and with negative parallax retinal disparity are suppressed by use of a variety of means.

## Figures

**SPECTRAL SENSITIVITIES OF THE L-, M-, AND S-CONES** in the human eye. The measurements are based on a light source at the cornea, so that the wavelength loss due to the cornea, lens, and other inert pigments of the eye plays a role in determining the sensitivity. Source: Stockman and MacLeod, 1993.


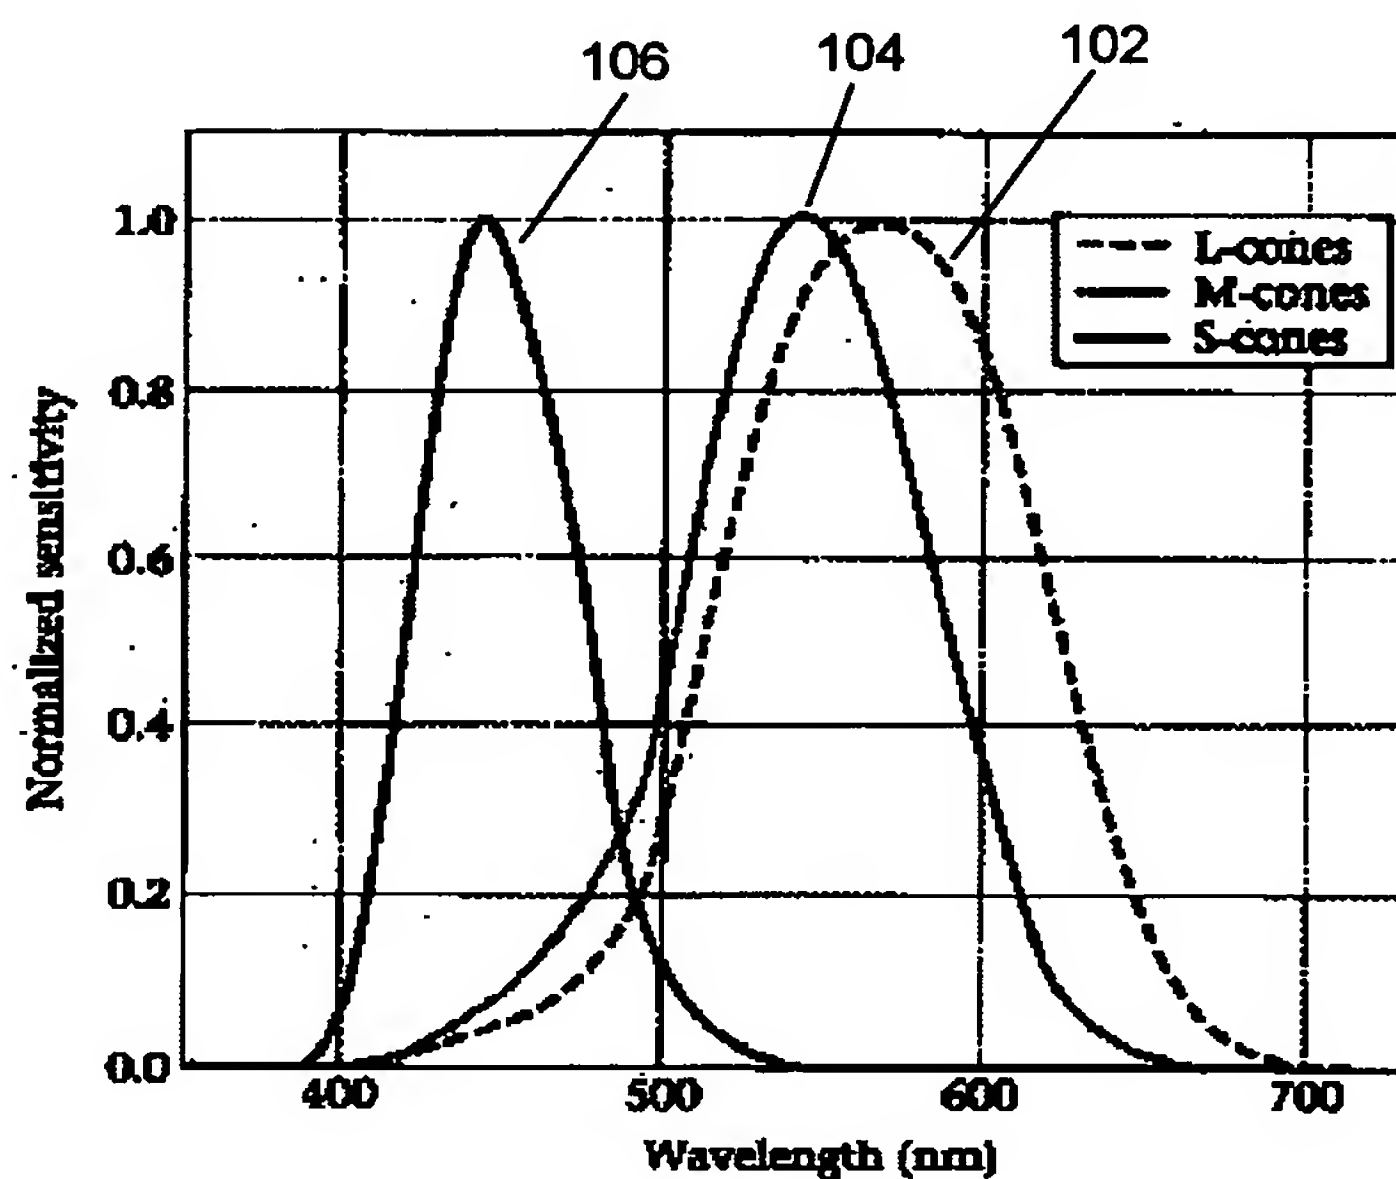


Figure 1

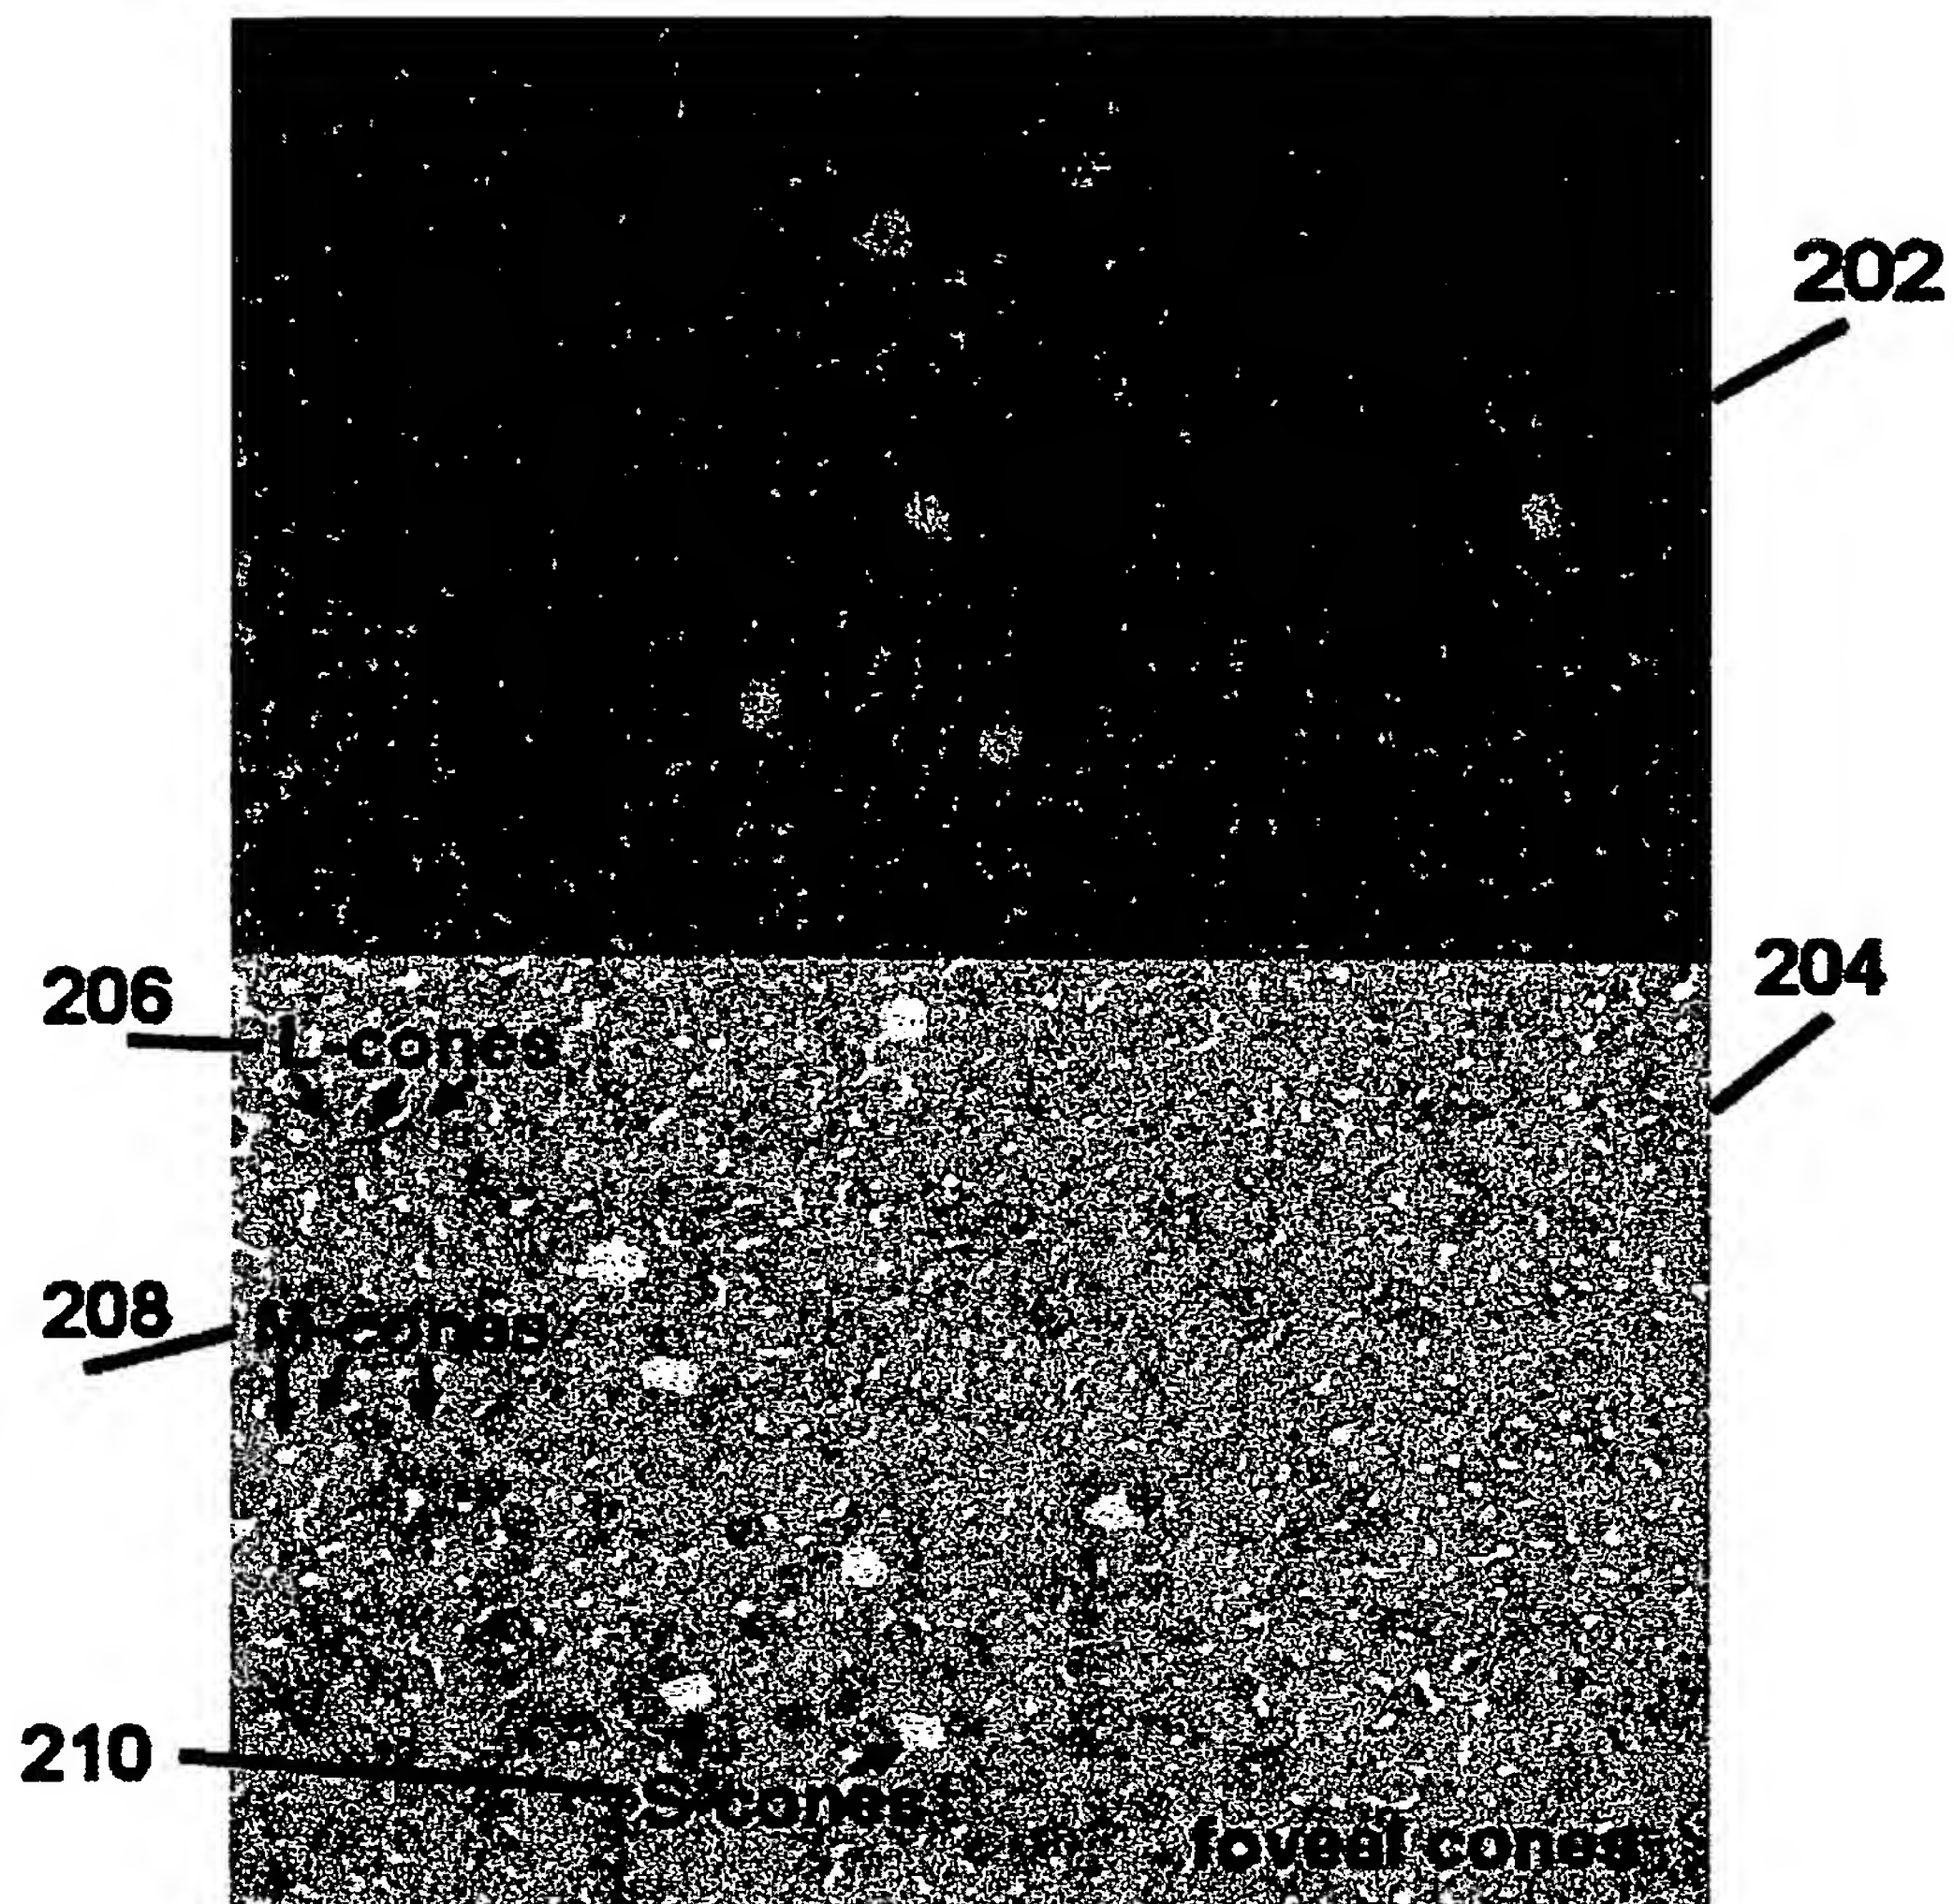

*Appearance of the cone mosaic in the fovea with and without the yellow macular pigment.*

**Figure 2**

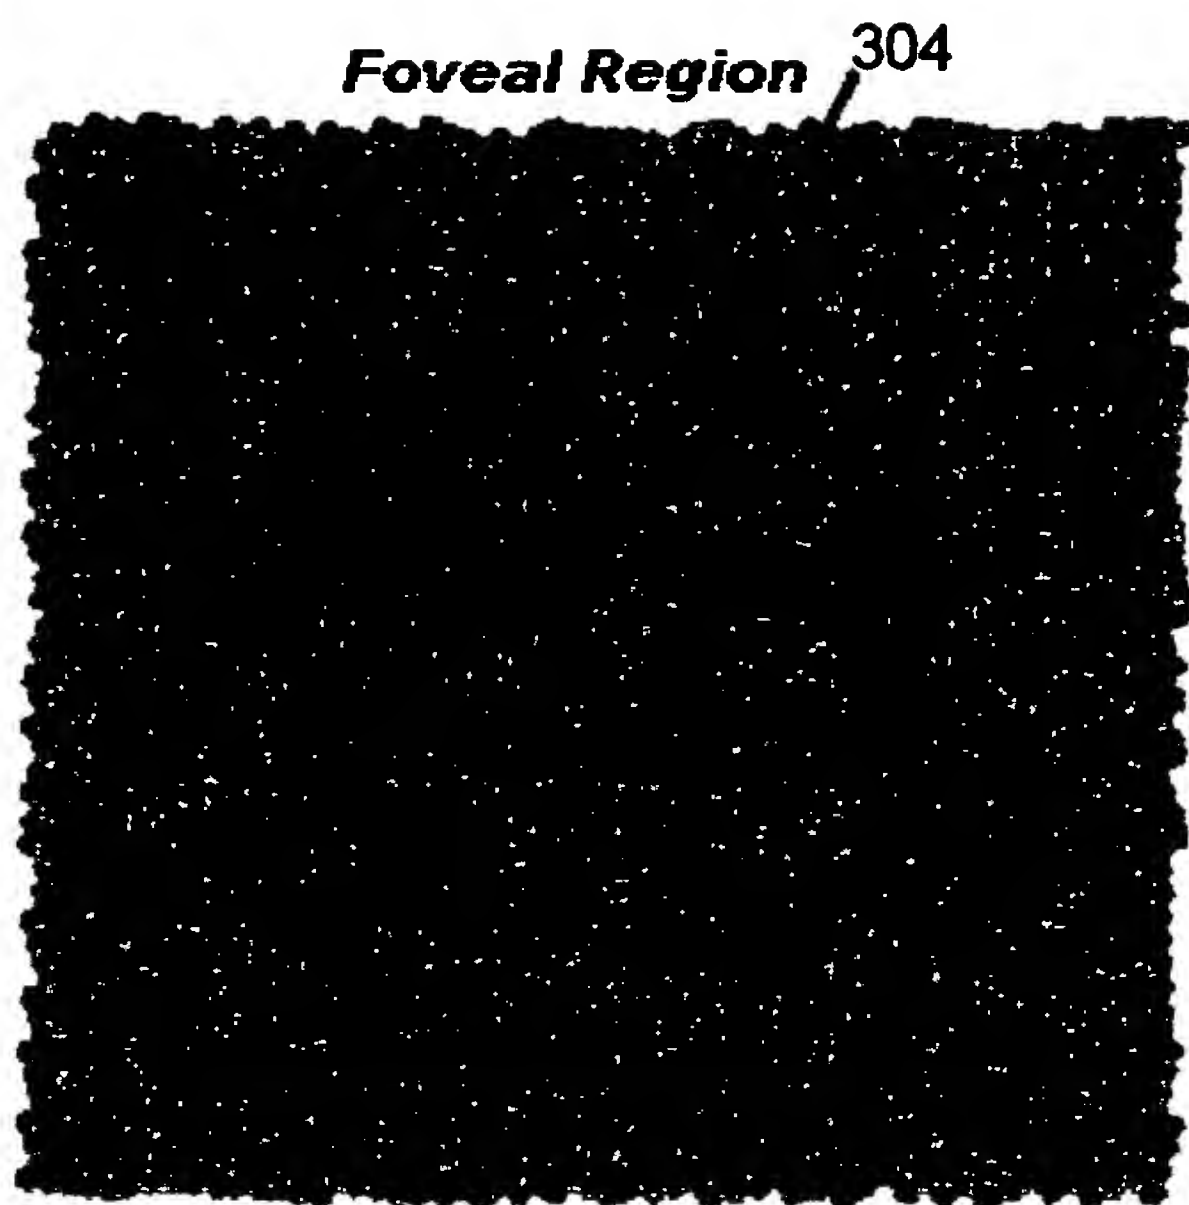
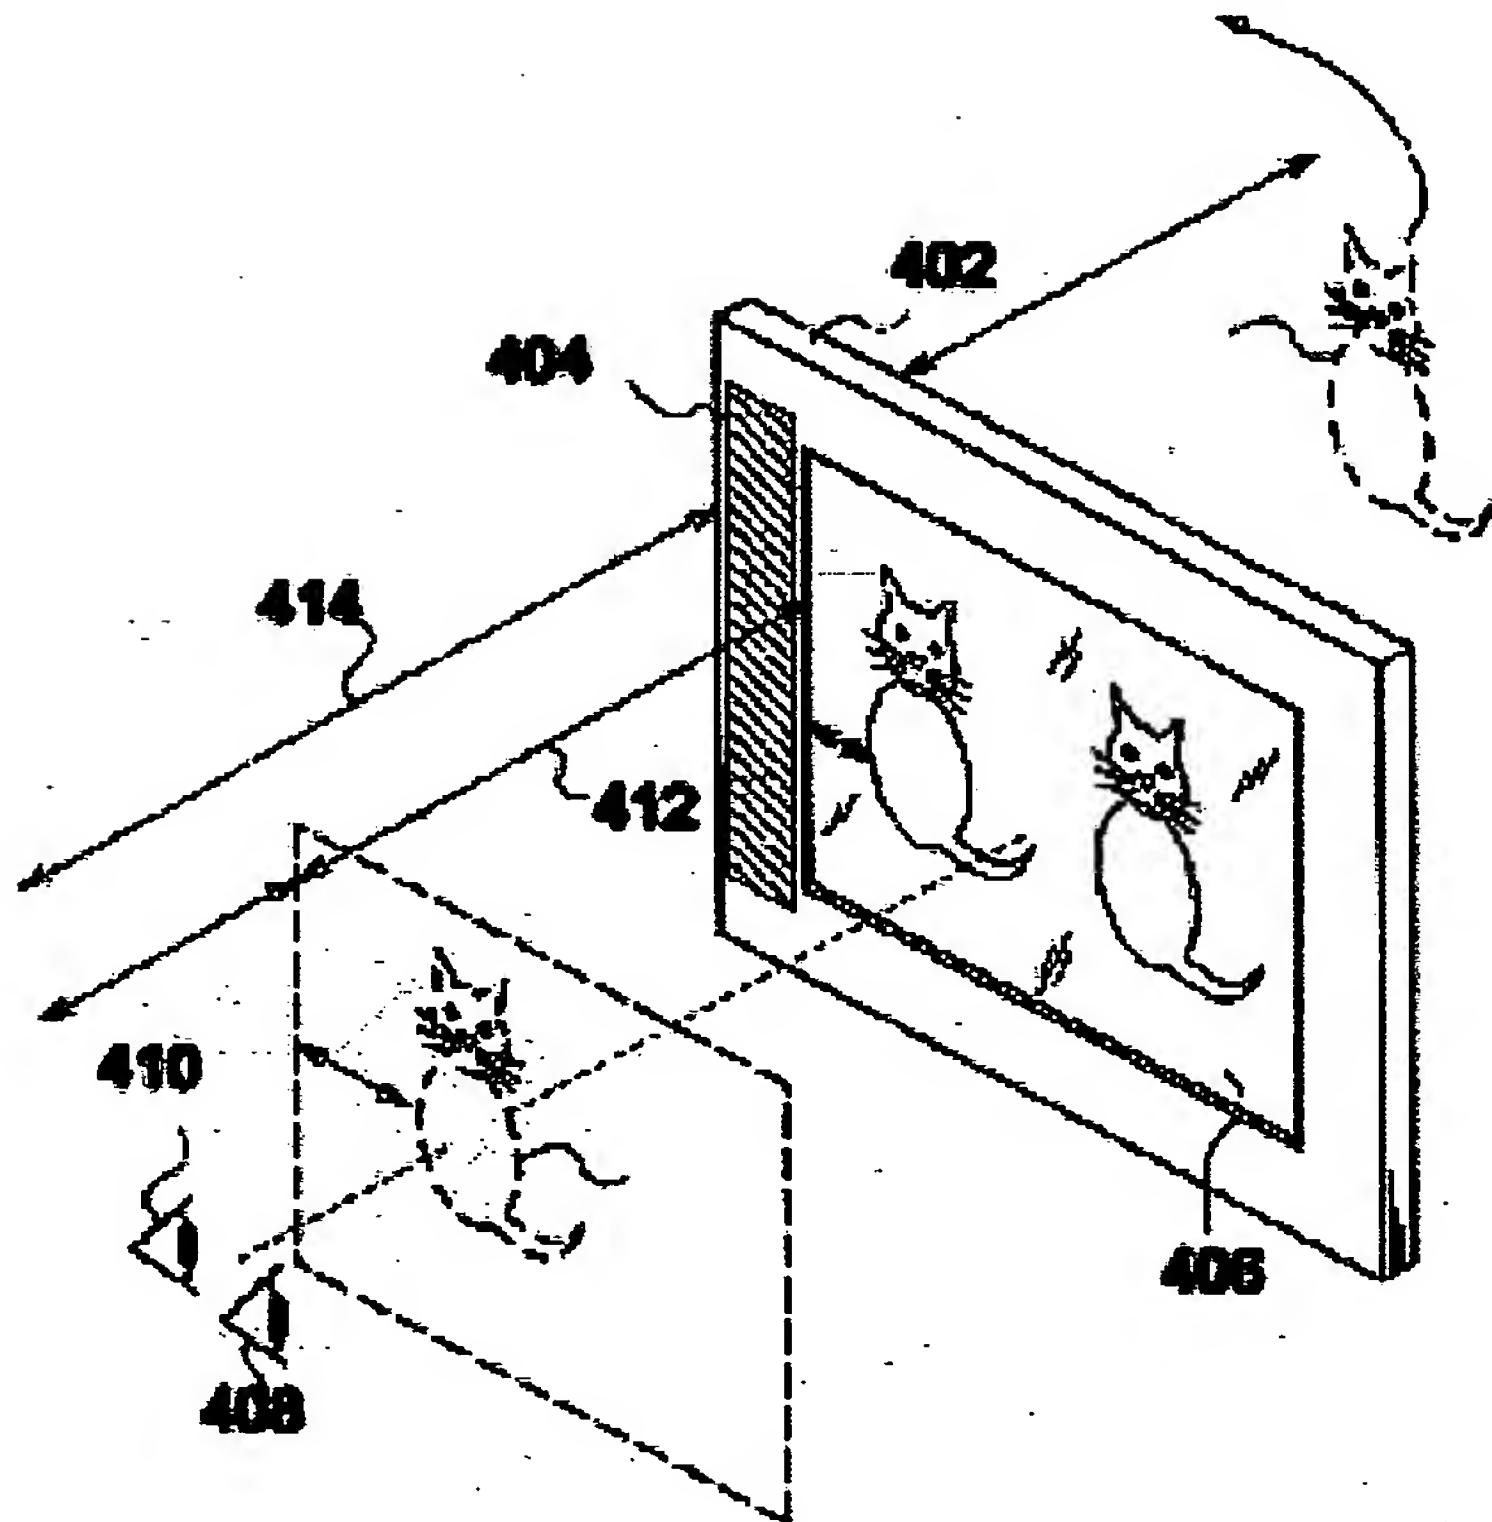


Figure 3

302 /

BEST AVAILABLE COPY



**Figure 4**